

FIG. 1

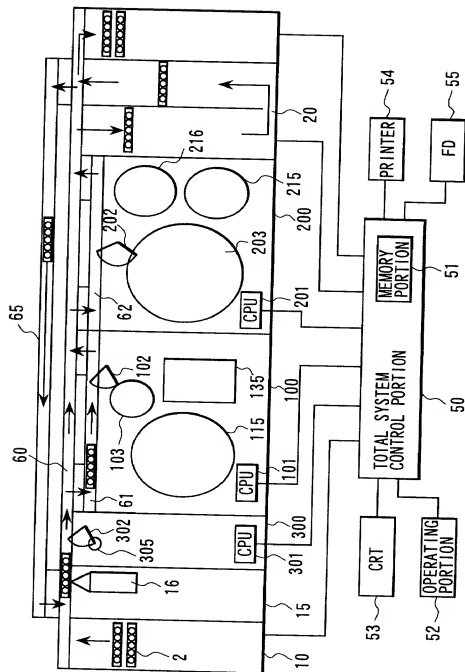


FIG.2

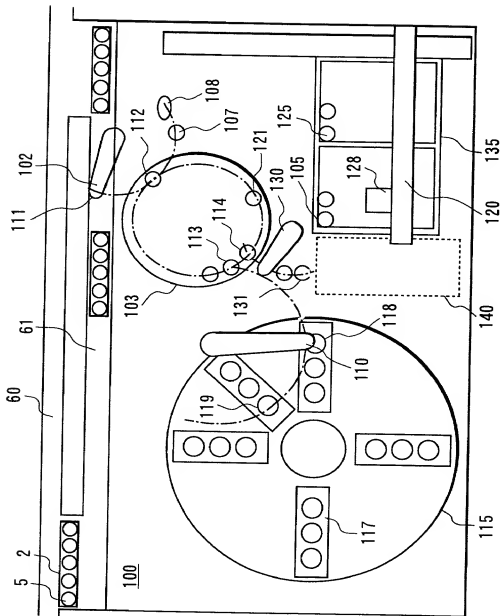


FIG.3

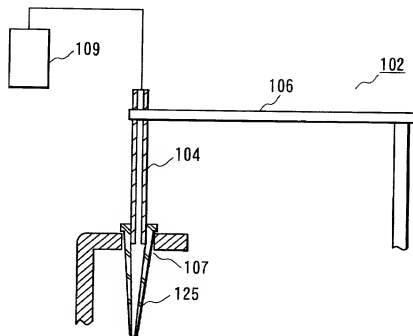


FIG.8

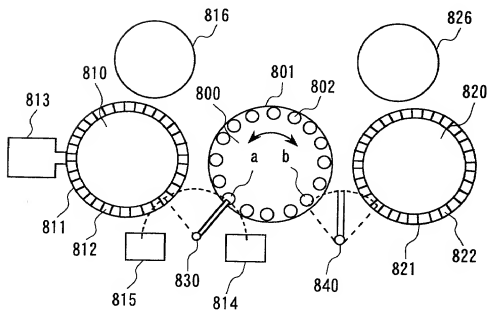


FIG. 5

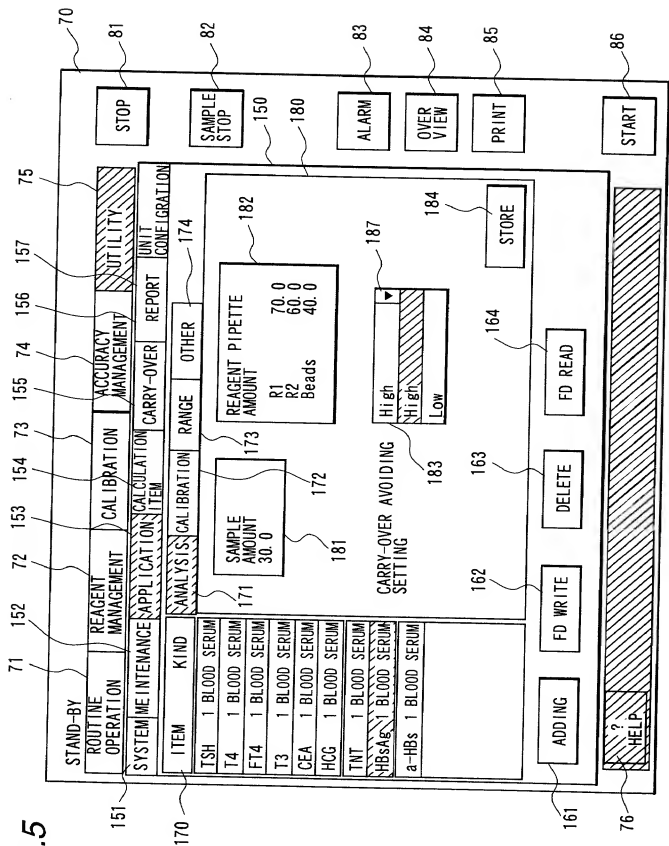


FIG. 6

70

71 72 73 74 75

STAND-BY ROUTINE OPERATION REAGENT MANAGEMENT CALIBRATION ACCURACY MANAGEMENT UTILITY

251

ITEM SELECTION

252

SAMPLE KIND BLOOD SERUM

253

1234567890

254

STANDARD

255

256

257

258

150

STOP

SAMPLE STOP

ALARM

OVER VIEW

PRINT

START

Sheet1 Sheet2 Sheet3 Sheet4 Sheet5

AST	Alb				Na K
AST	Alb				
AST	Alb				
AST	Alb				

PRECEDING SAMPLE

FOLLOWING SAMPLE

REGISTER

?

HELP

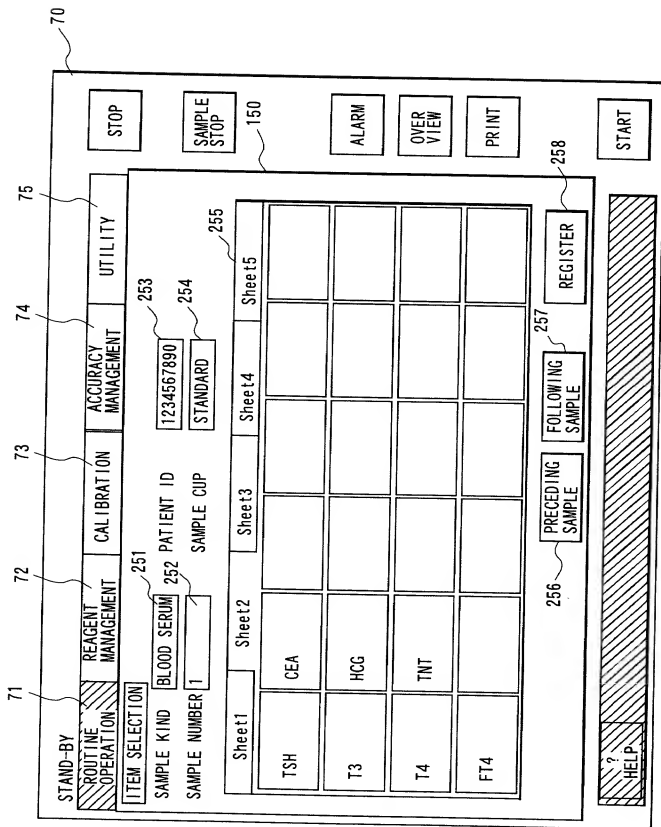


FIG.9

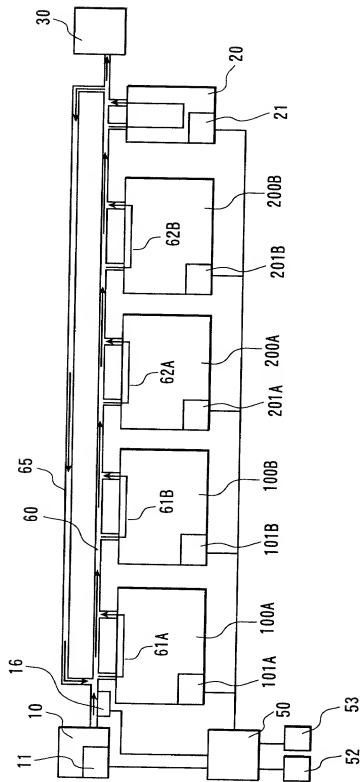


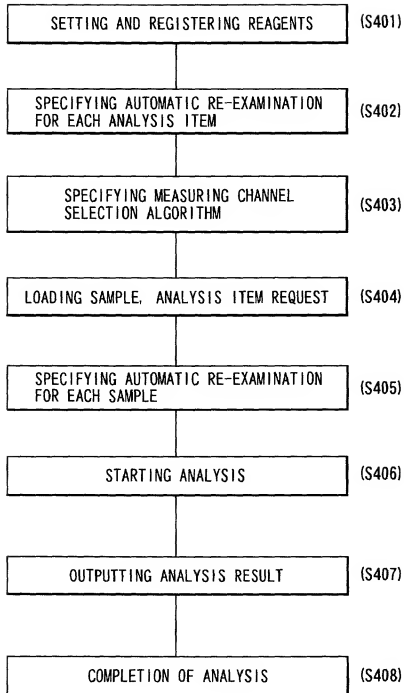
FIG.10

FIG. 11A

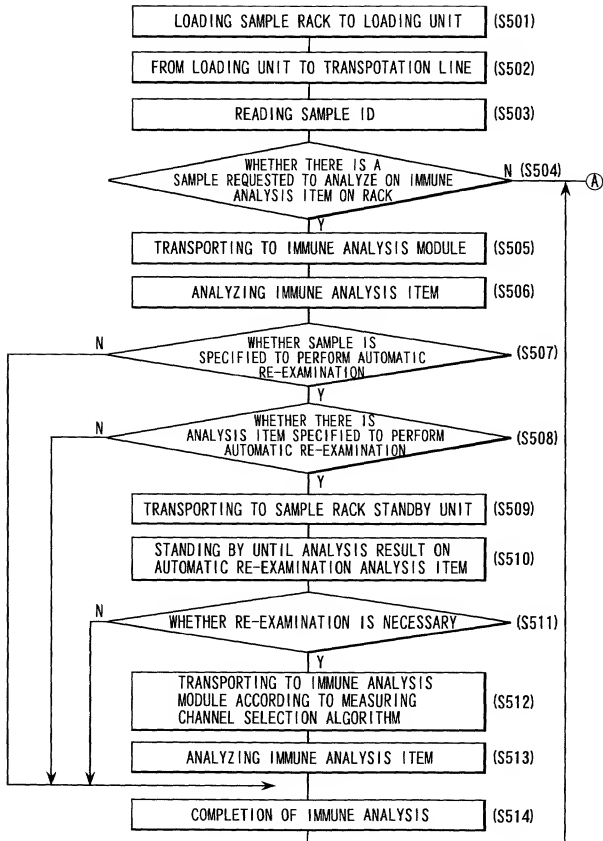


FIG.11B

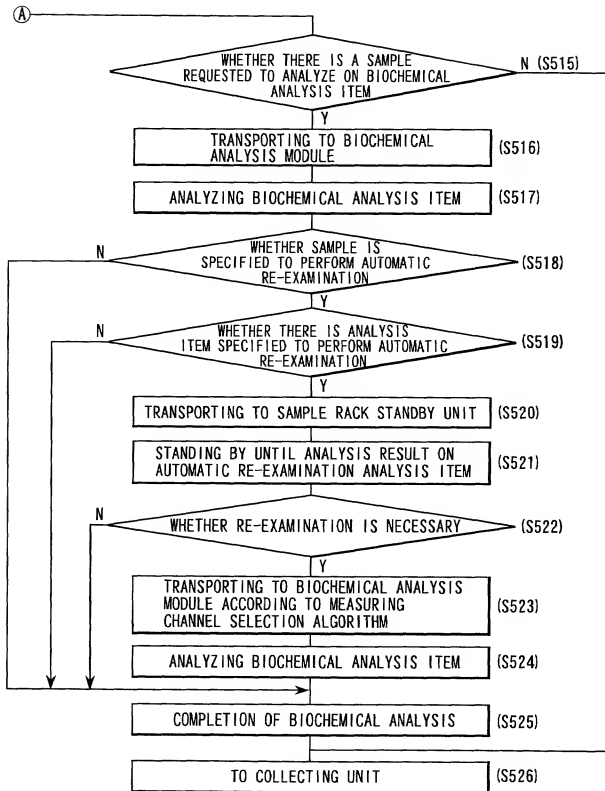


FIG. 12

